Data File C:\CHEM32\1\DATA\EC 2870 ANALYSIS
Sample Name:

==========

Acq. Operator : lida
Location : Vial 1
Injection Date : 23.02.2022 22:35:38
Acq. Method :
Analysis Method : C:\CHEM32\1\METHODS\VALIDATION.M
Last changed : 21.09.2022 14:15:41

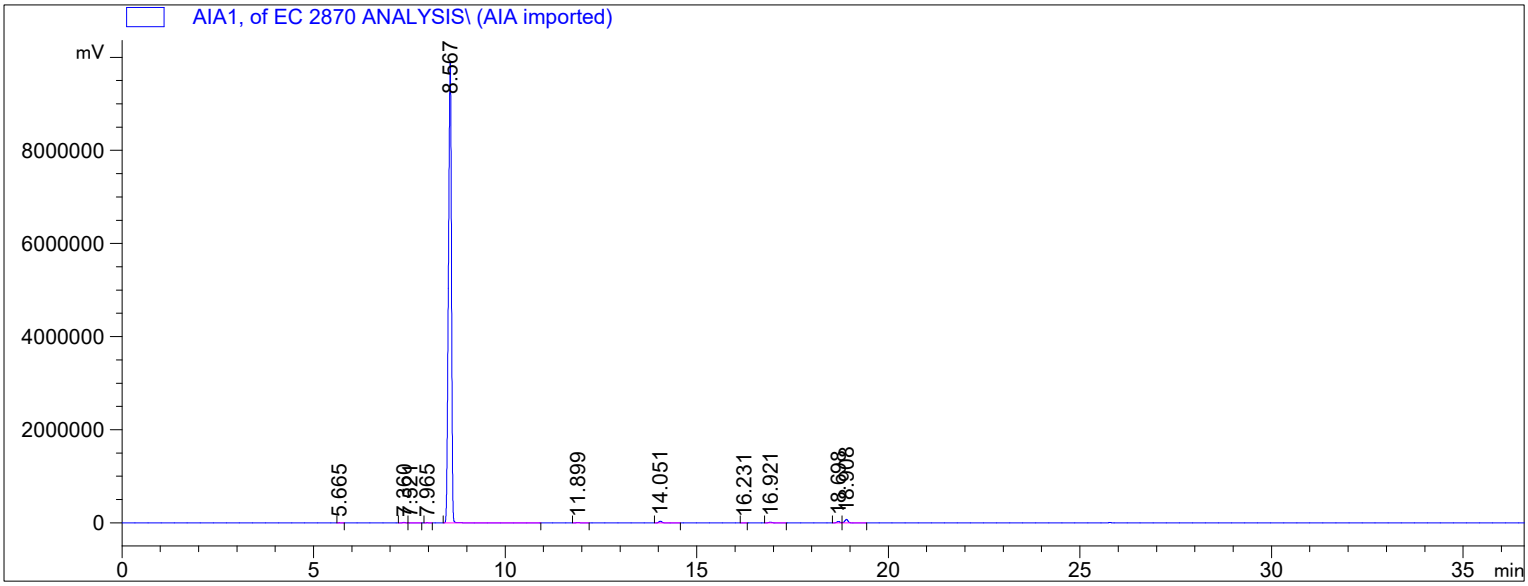

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : 21 September 2022 г. 14:13:16
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: AIA1,

Peak #	RetTime [min]	Type		Width [min]	Area [mV*s]	Area %	Name
1	5.665	BB		5.44e-4	3021.70190	0.00830	acetaldehyde
2	7.521	BB		9.33e-4	3572.16211	0.00982	ethyl acetate
3	7.611			0.0000	0.00000	0.00000	acetal
4	7.965	BB		8.89e-4	4731.48340	0.01300	methanol
5	8.567	BB	I	1.47e-3	3.57904e7	98.35918	ethanol
6	11.445			0.0000	0.00000	0.00000	butan-2-ol
7	11.899	BB		1.34e-3	1.91972e4	0.05276	propan-1-ol
8	14.051	BB		1.33e-3	1.19137e5	0.32741	2-methylpropan-1-ol
9	16.231	BB		1.28e-3	401.14813	0.00110	butan-1-ol
10	16.921	BB	I	1.37e-3	5.30284e4	0.14573	4-methylpentan-2-ol
11	18.698	BB		1.34e-3	9.73665e4	0.26758	3-methylbutan-1-ol
12	18.908	BB		1.49e-3	2.73425e5	0.75143	2-methylbutan-1-ol
Totals :					3.63642e7	99.9363	

3 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found
Warning : Elution order of calibrated compounds may have changed

Data File C:\CHEM32\1\DATA\EC 2870 ANALYSIS
Sample Name:

==========

*** End of Report ***

Data File C:\CHEM32\1\DATA\EC 2870 ANALYSIS
Sample Name:

==========

Acq. Operator : lida
Location : Vial 1
Injection Date : 23.02.2022 23:18:34
Acq. Method :
Analysis Method : C:\CHEM32\1\METHODS\VALIDATION.M
Last changed : 21.09.2022 14:15:41

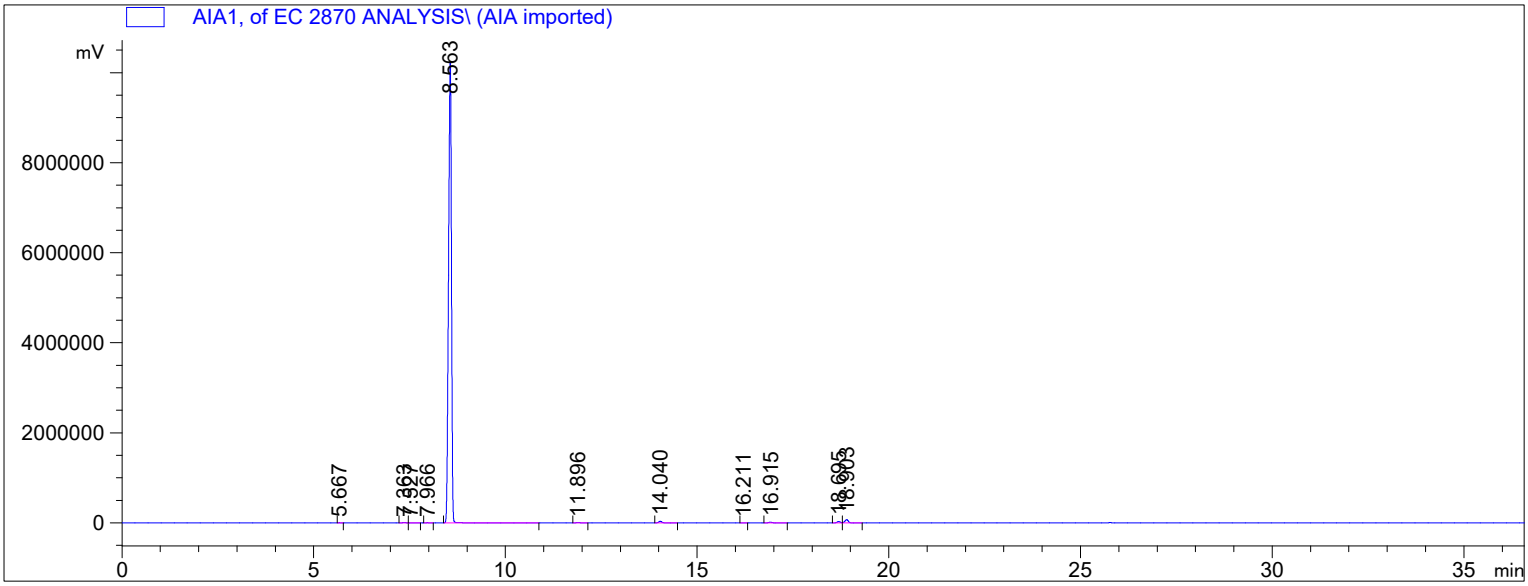

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : 21 September 2022 г. 14:13:16
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: AIA1,

Peak #	RetTime [min]	Type	Width [min]	Area [mV*s]	Area %	Name
1	5.667	BB	5.67e-4	3016.62476	0.00825	acetaldehyde
2	7.527	BB	9.22e-4	3510.41089	0.00960	ethyl acetate
3	7.611		0.0000	0.00000	0.00000	acetal
4	7.966	BB	9.11e-4	4789.12158	0.01309	methanol
5	8.563	BB I	1.42e-3	3.59750e7	98.36321	ethanol
6	11.445		0.0000	0.00000	0.00000	butan-2-ol
7	11.896	BB	1.38e-3	1.92304e4	0.05258	propan-1-ol
8	14.040	BB	1.33e-3	1.19557e5	0.32689	2-methylpropan-1-ol
9	16.211	BB	1.31e-3	415.73950	0.00114	butan-1-ol
10	16.915	BB I	1.37e-3	5.23680e4	0.14319	4-methylpentan-2-ol
11	18.695	BB	1.34e-3	9.79474e4	0.26781	3-methylbutan-1-ol
12	18.903	BB	1.49e-3	2.74448e5	0.75040	2-methylbutan-1-ol
Totals :				3.65503e7	99.9362	

3 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found
Warning : Elution order of calibrated compounds may have changed

Data File C:\CHEM32\1\DATA\EC 2870 ANALYSIS
Sample Name:

==========

*** End of Report ***

Data File C:\CHEM32\1\DATA\EC 2870 ANALYSIS
Sample Name:

==========

Acq. Operator : lida
Location : Vial 1
Injection Date : 24.02.2022 0:01:29
Acq. Method :
Analysis Method : C:\CHEM32\1\METHODS\VALIDATION.M
Last changed : 21.09.2022 14:15:41

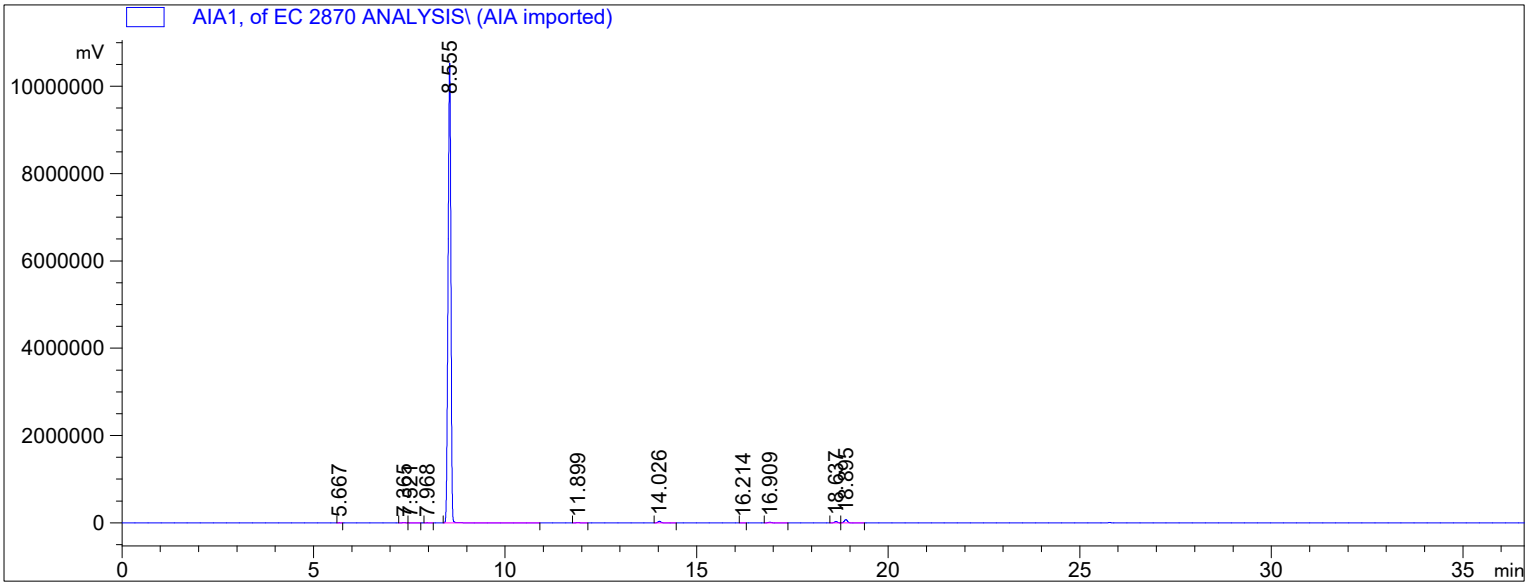

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : 21 September 2022 г. 14:13:16
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: AIA1,

Peak #	RetTime [min]	Type	Width [min]	Area [mV*s]	Area %	Name
1	5.667	BB	5.78e-4	3031.40967	0.00830	acetaldehyde
2	7.521	BB	9.33e-4	3434.33887	0.00941	ethyl acetate
3	7.611		0.0000	0.00000	0.00000	acetal
4	7.968	BB	9.22e-4	4796.05859	0.01314	methanol
5	8.555	BB I	1.37e-3	3.59094e7	98.36202	ethanol
6	11.445		0.0000	0.00000	0.00000	butan-2-ol
7	11.899	BB	1.39e-3	1.92007e4	0.05259	propan-1-ol
8	14.026	BB	1.33e-3	1.19147e5	0.32636	2-methylpropan-1-ol
9	16.214	BB	1.28e-3	409.46075	0.00112	butan-1-ol
10	16.909	BB I	1.38e-3	5.21384e4	0.14282	4-methylpentan-2-ol
11	18.637	BB	1.34e-3	9.83043e4	0.26927	3-methylbutan-1-ol
12	18.895	BB	1.49e-3	2.74147e5	0.75094	2-methylbutan-1-ol
Totals :				3.64841e7	99.9360	

3 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found
Warning : Elution order of calibrated compounds may have changed

Data File C:\CHEM32\1\DATA\EC 2870 ANALYSIS
Sample Name:

==========

*** End of Report ***