


Sample Name: Moscoviya - 95

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                Location : Vial 101
Injection Date  : 14.06.2022 14:47:57      Inj      : 1
                                           Inj Volume : 1 µl

Acq. Method     : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed    : 08.06.2022 14:22:28
Analysis Method  : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed    : 20.06.2022 14:30:13
Method Info     : 25.06.2019 H2
=====

```

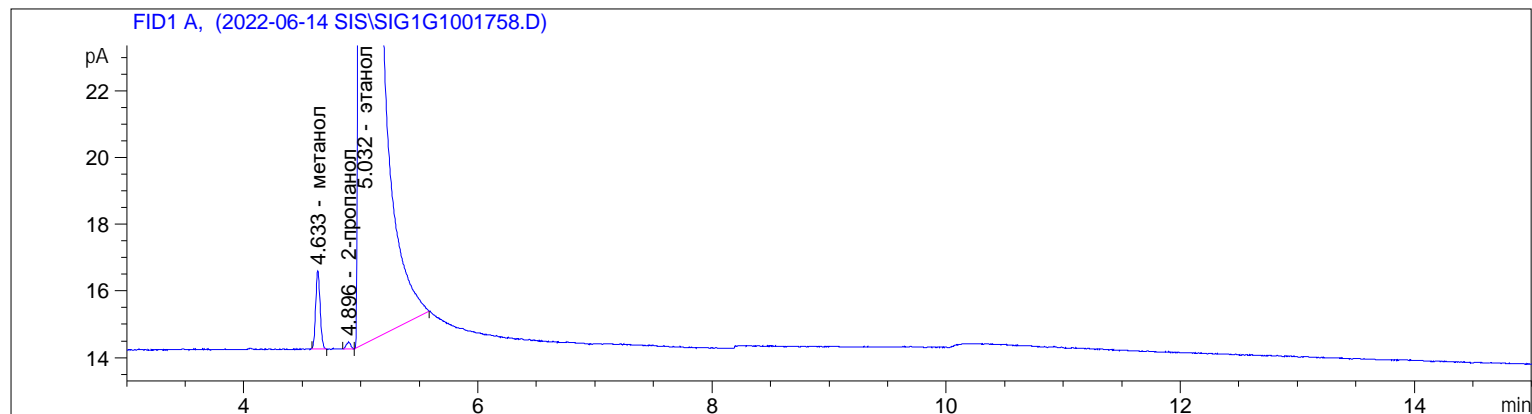

```

=====
External Standard Report
=====

```

```

Sorted By       : Signal
Calib. Data Modified : 20.06.2022 14:28:58
Multiplier:     : 1.0000
Dilution:       : 1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: FID1 A,

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [мг/дм3]	Grp	Name
3.482		-	-	-		ацетальдегид
4.075		-	-	-		метилацетат
4.549		-	-	-		этилацетат
4.633	BB	6.31566	2.26991e-4	1.43360e-3		метанол
4.896	BV	5.55516e-1	1.50399	8.35488e-1		2-пропанол
5.032	VB S	1.89793e5	1.98117e-4	37.60121		этанол
7.057		-	-	-		1-пропанол
8.778		-	-	-		изобутиловый спирт
11.063		-	-	-		1-бутанол
13.337		-	-	-		изоамиловый спирт

```
Totals : 38.43813
```

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

Sample Name: Moscoviya - 95

=====

\*\*\* End of Report \*\*\*