


Sample Name: konak

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                Location : Vial 101
Injection Date  : 14.06.2022 13:13:21      Inj      : 1
                                                Inj Volume : 1 µl

Acq. Method    : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed   : 08.06.2022 14:22:28
Analysis Method : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed   : 20.06.2022 14:30:13
Method Info    : 25.06.2019 H2
=====

```

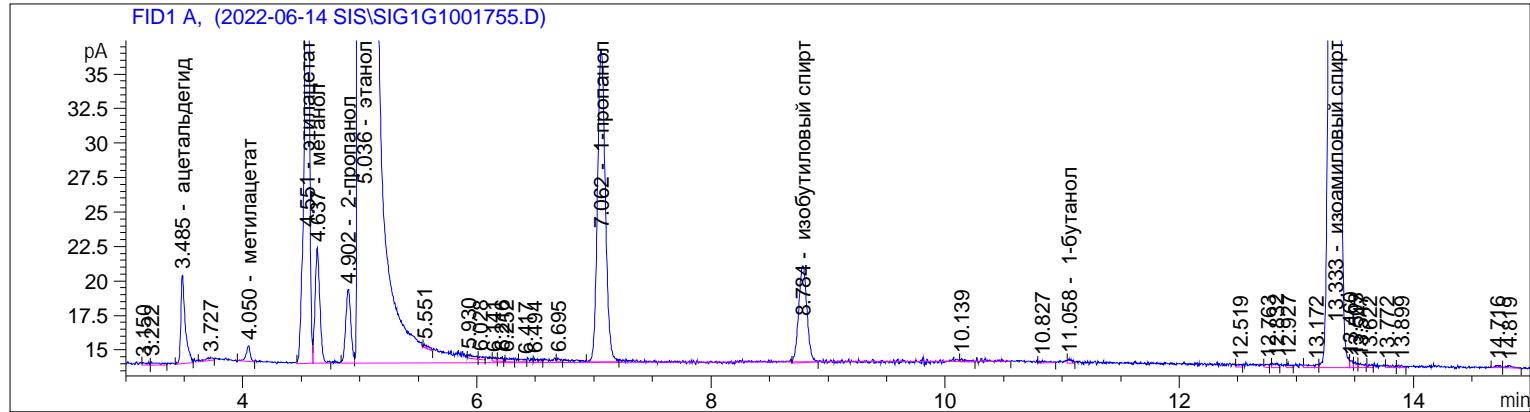

```

=====
External Standard Report
=====

```

```

Sorted By           : Signal
Calib. Data Modified : 20.06.2022 14:28:58
Multiplier          : 1.0000
Dilution            : 1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: FID1 A,

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [мг/дм3]	Grp	Name
3.485	VV	16.95651	2.29312	38.88323		ацетальдегид
4.050	BV	2.80551	2.62726	7.37081		метилацетат
4.551	BV	128.33510	1.55917	200.09636		этилацетат
4.637	VB	24.14906	2.26991e-4	5.48162e-3		метанол
4.902	BV	16.46674	1.50399	24.76574		2-пропанол
5.036	VB S	2.16074e5	1.98117e-4	42.80782		этанол
7.062	VV T	104.56990	1.10088	115.11874		1-пропанол
8.784	PV T	34.57939	1.00230	34.65885		изобутиловый спирт
11.058	BV	7.03571e-1	1.00560	7.07514e-1		1-бутанол
13.333	VV	854.57062	9.73467e-1	831.89621		изоамиловый спирт

```
Totals : 1296.31075
```

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Sample Name: konak

=====

*** End of Report ***