


```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                      Location : Vial 101
Injection Date  : 14.06.2022 14:47:57           Inj      : 1
                                                    Inj Volume : 1 µl

Acq. Method     : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed    : 08.06.2022 14:22:28
Analysis Method  : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed    : 20.06.2022 14:45:03
                  (modified after loading)
Method Info     : 25.06.2019 H2
  
```

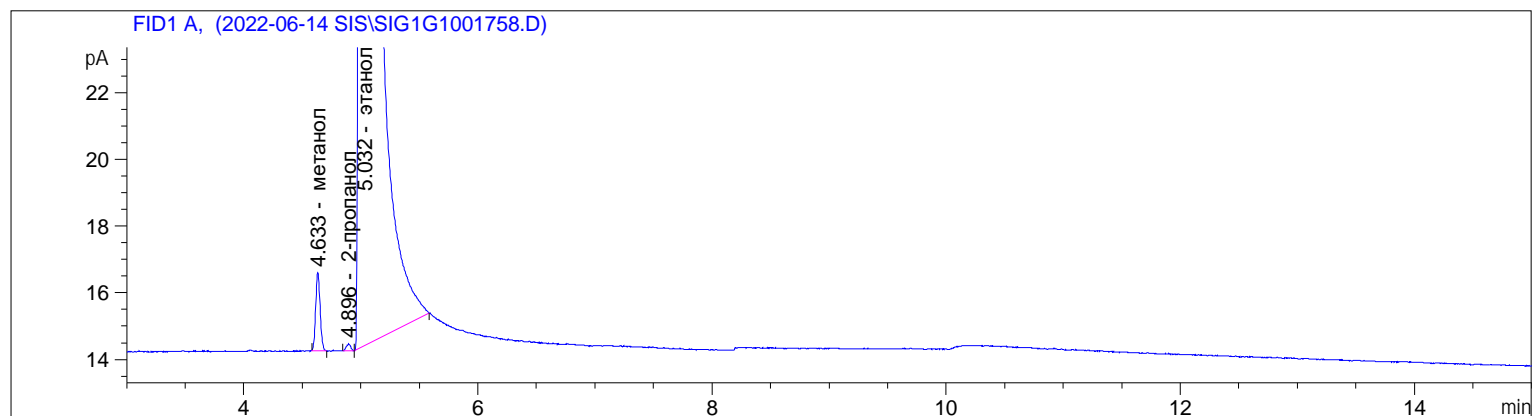

Internal Standard Report

```

Sorted By      : Signal
Calib. Data Modified : 20 June 2022 г. 14:45:03
Multiplier:    : 1.0000
Dilution:     : 1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Sample ISTD Information:

ISTD #	ISTD Amount мг/л безво	Name
1	7.89270e5	этанол

Signal 1: FID1 A,

RetTime [min]	Type	ISTD used	Area [pA*s]	Amt/Area ratio	Amount мг/л безво	Grp	Name
3.482		1	-	-	-		ацетальдегид
4.075		1	-	-	-		метилацетат
4.549		1	-	-	-		этилацетат
4.633	BV	1	6.31566	1.45165e-4	3.81264e-3		метанол
4.896	BV	1	5.55516e-1	9.61827e-1	2.22197		2-пропанол
5.032	VB S I	1	1.89793e5	1.00000	7.89270e5		этанол
7.057		1	-	-	-		1-пропанол
8.778		1	-	-	-		изобутиловый спирт
11.063		1	-	-	-		1-бутанол
13.337		1	-	-	-		изоамиловый спирт

Sample Name: Moscoviya - 95

Totals without ISTD(s) : 2.22578

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====

*** End of Report ***