


Sample Name: konak

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                Location : Vial 101
Injection Date  : 14.06.2022 13:13:21      Inj      : 1
                                           Inj Volume : 1 µl

Acq. Method     : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed    : 08.06.2022 14:22:28
Analysis Method : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed    : 20.06.2022 14:45:03
                 (modified after loading)
Method Info     : 25.06.2019 H2
=====

```

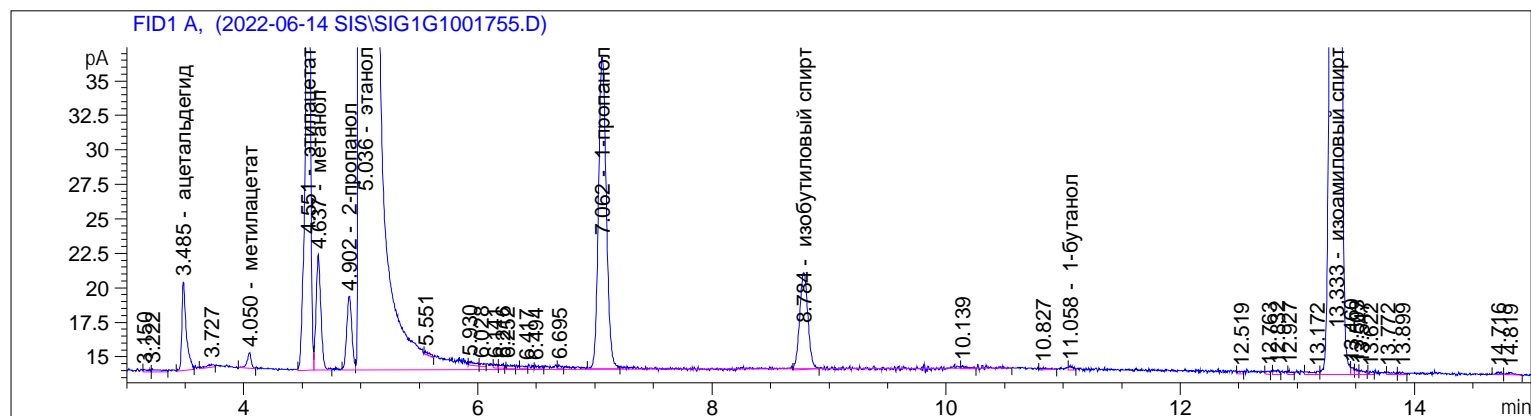

```

=====
Internal Standard Report
=====

```

```

Sorted By      : Signal
Calib. Data Modified : 20 June 2022 г. 14:45:03
Multiplier:    : 1.0000
Dilution:      : 1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Sample ISTD Information:

ISTD #	ISTD Amount мг/л безво	Name
1	7.89270e5	этанол

Signal 1: FID1 A,

RetTime [min]	Type	ISTD used	Area [pA*s]	Amt/Area ratio	Amount мг/л безво	Grp	Name
3.485	VV	1	16.95651	1.46649	90.83207		ацетальдегид
4.050	BV	1	2.80551	1.68018	17.21838		метилацетат
4.551	BV	1	128.33510	9.97119e-1	467.42943		этилацетат
4.637	VB	1	24.14906	1.45165e-4	1.28052e-2		метанол
4.902	BV	1	16.46674	9.61827e-1	57.85330		2-пропанол
5.036	VB S I	1	2.16074e5	1.00000	7.89270e5		этанол
7.062	VV T	1	104.56990	7.04032e-1	268.91986		1-пропанол
8.784	PV T	1	34.57939	6.40988e-1	80.96382		изобутиловый спирт
11.058	BV	1	7.03571e-1	6.43102e-1	1.65277		1-бутанол
13.333	VV	1	854.57062	6.22550e-1	1943.32758		изоамиловый спирт

Sample Name: konak

Totals without ISTD(s) : 2928.21002

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

=====
*** End of Report ***