


Sample Name: calvados

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                Location : Vial 101
Injection Date  : 14.06.2022 12:38:52      Inj       : 1
                                           Inj Volume: 1 µl

Acq. Method     : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed    : 08.06.2022 14:22:28
Analysis Method : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed    : 20.06.2022 14:45:03
                 (modified after loading)
Method Info     : 25.06.2019 H2
    
```

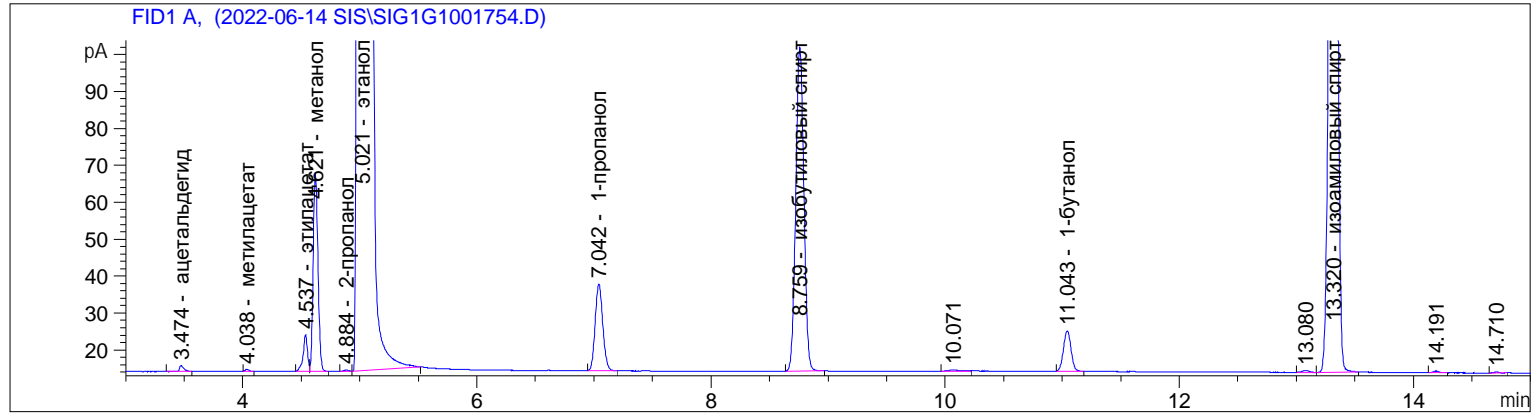

Internal Standard Report

```

Sorted By           : Signal
Calib. Data Modified : 20 June 2022 г. 14:45:03
Multiplier          : 1.0000
Dilution            : 1.0000
Use Multiplier & Dilution Factor with ISTDs
    
```

Sample ISTD Information:

ISTD #	ISTD Amount (мг/л безво)	Name
1	7.89270e5	этанол

Signal 1: FID1 A,

RetTime [min]	Type	ISTD used	Area [pA*s]	Amt/Area ratio	Amount (мг/л безво)	Grp	Name
3.474	VB	1	4.07187	1.46649	22.57551		ацетальдегид
4.038	VB	1	1.18820	1.68018	7.54764		метилацетат
4.537	BV	1	25.57652	9.97119e-1	96.41677		этилацетат
4.621	VB	1	151.90663	1.45165e-4	8.33687e-2		метанол
4.884	BV	1	9.12119e-1	9.61827e-1	3.31675		2-пропанол
5.021	VB S I	1	2.08767e5	1.00000	7.89270e5		этанол
7.042	VB	1	106.25713	7.04032e-1	282.82301		1-пропанол
8.759	VB	1	422.23059	6.40988e-1	1023.20787		изобутиловый спирт
11.043	VB	1	49.33747	6.43102e-1	119.95573		1-бутанол
13.320	VB	1	1356.46594	6.22550e-1	3192.62153		изоамиловый спирт

Sample Name: calvados

Totals without ISTD(s) : 4748.54816

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

=====

*** End of Report ***