


Sample Name: 2

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                Location : Vial 101
Injection Date  : 14.06.2022 15:19:06      Inj      : 1
                                                Inj Volume : 1 µl

Acq. Method     : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed    : 08.06.2022 14:22:28
Analysis Method : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed    : 08.06.2022 14:22:28
Method Info     : 25.06.2019 H2
=====

```

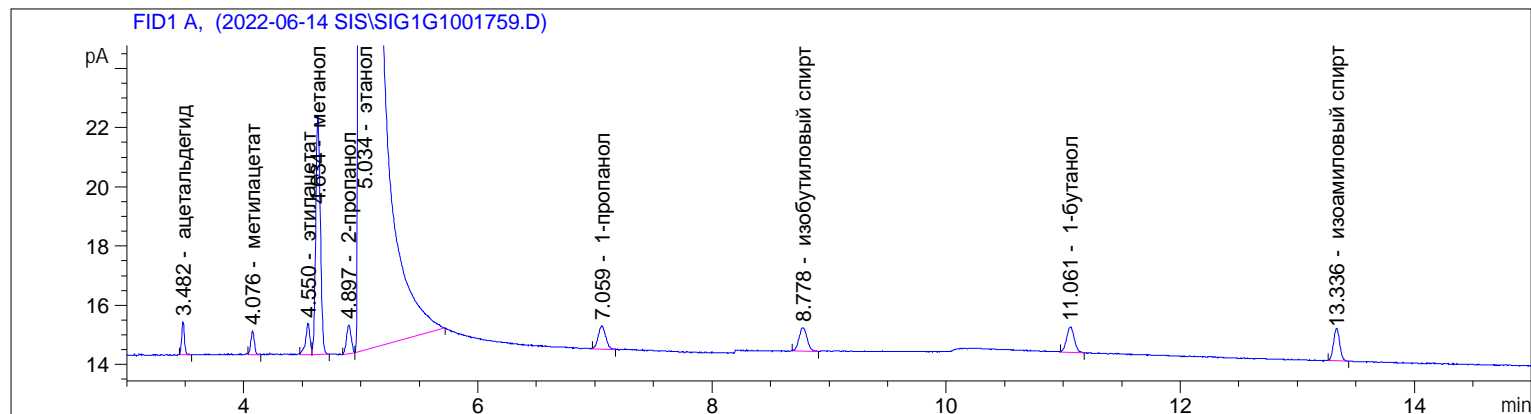

```

=====
External Standard Report
=====

```

```

Sorted By           : Signal
Calib. Data Modified : Wednesday, June 08, 2022 3:18:42 PM
Multiplier:         : 1.0000
Dilution:           : 1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: FID1 A,

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [мг/дм3]	Grp	Name
3.482	BB	1.87640	2.55080	4.78631		ацетальдегид
4.076	BB	1.61751	2.90136	4.69298		метилацетат
4.550	BV	2.73721	1.62350	4.44387		этилацетат
4.634	VB	22.07565	2.32182e-4	5.12558e-3		метанол
4.897	BV	2.66154	1.55854	4.14812		2-пропанол
5.034	VB S	1.92774e5	2.09954e-4	40.47365		этанол
7.059	BB	3.41357	1.15980	3.95907		1-пропанол
8.778	BB	3.85656	1.03917	4.00763		изобутиловый спирт
11.061	BB	3.86672	1.02306	3.95589		1-бутанол
13.336	BB	4.02269	9.80381e-1	3.94377		изоамиловый спирт

```
Totals : 74.41641
```

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Sample Name: 2

=====

*** End of Report ***