


Sample Name: Moscoviya - 95

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                Location : Vial 101
Injection Date  : 14.06.2022 14:47:57      Inj      : 1
                                           Inj Volume : 1 µl

Acq. Method     : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed    : 08.06.2022 14:22:28
Analysis Method  : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed    : 08.06.2022 14:22:28
Method Info     : 25.06.2019 H2
  
```

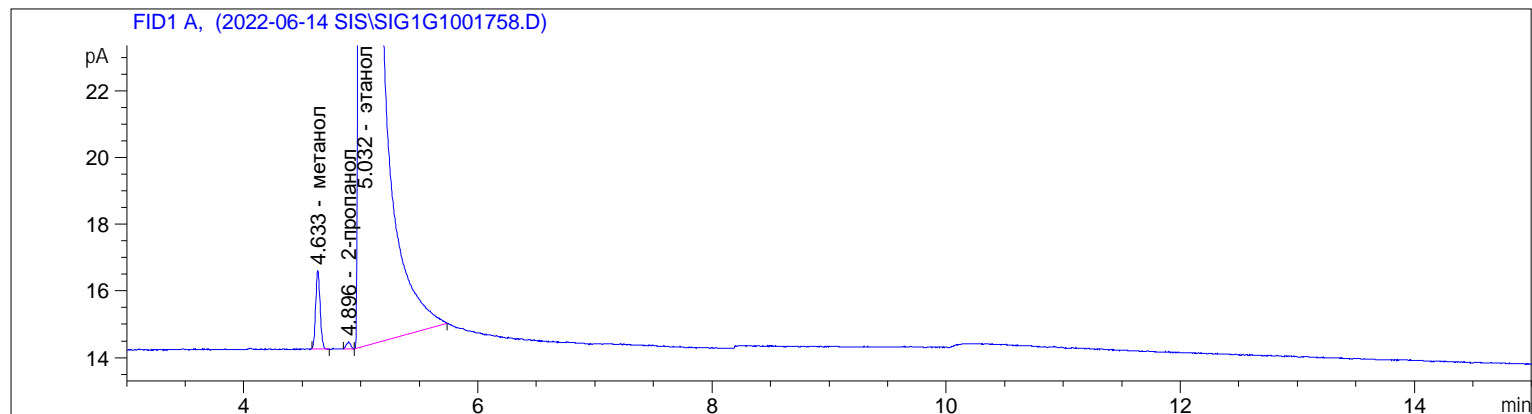

```

=====
External Standard Report
=====
  
```

```

Sorted By      : Signal
Calib. Data Modified : Wednesday, June 08, 2022 3:18:42 PM
Multiplier:    : 1.0000
Dilution:     : 1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: FID1 A,

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [мг/дм3]	Grp	Name
3.467		-	-	-		ацетальдегид
4.059		-	-	-		метилацетат
4.530		-	-	-		этилацетат
4.633	BB	6.31234	2.17309e-4	1.37173e-3		метанол
4.896	BV	5.52898e-1	1.55215	8.58178e-1		2-пропанол
5.032	VB S	1.89805e5	2.09954e-4	39.85030		этанол
7.029		-	-	-		1-пропанол
8.740		-	-	-		изобутиловый спирт
11.026		-	-	-		1-бутанол
13.306		-	-	-		изоамиловый спирт

```
Totals : 40.70985
```

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

Sample Name: Moscoviya - 95

=====

*** End of Report ***