


Sample Name: konak

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                      Location : Vial 101
Injection Date  : 14.06.2022 13:13:21           Inj       : 1
                                                    Inj Volume: 1 µl

Acq. Method     : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed    : 08.06.2022 14:22:28
Analysis Method  : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed    : 08.06.2022 14:22:28
Method Info     : 25.06.2019 H2
=====

```

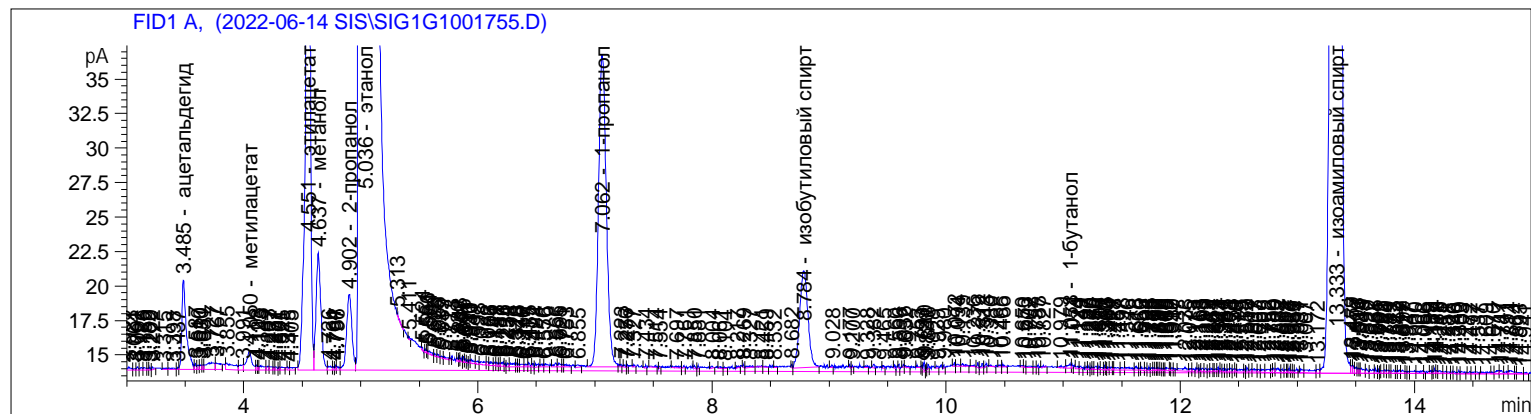

```

=====
External Standard Report
=====

```

```

Sorted By       : Signal
Calib. Data Modified : Wednesday, June 08, 2022 3:18:42 PM
Multiplier:     : 1.0000
Dilution:       : 1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: FID1 A,

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [мг/дм3]	Grp	Name
3.485	VV	17.58351	2.65405	46.66744		ацетальдегид
4.050	VV	4.13836	2.93509	12.14645		метилацетат
4.551	BV	129.27979	1.68307	217.58722		этилацетат
4.637	VV	24.71154	2.32818e-4	5.75329e-3		метанол
4.902	VV	17.55067	1.55997	27.37843		2-пропанол
5.036	VBAS	2.16195e5	2.09954e-4	45.39102		этанол
7.062	VV T	104.47670	1.17396	122.65134		1-пропанол
8.784	VV T	34.64483	1.04800	36.30766		изобутиловый спирт
11.058	VV T	5.61411e-1	9.31777e-1	5.23110e-1		1-бутанол
13.333	PV T	854.89056	1.01082	864.13856		изоамиловый спирт

```
Totals : 1372.79698
```

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Sample Name: konak

=====

\*\*\* End of Report \*\*\*