


Sample Name: pB

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                Location : Vial 101
Injection Date  : 14.06.2022 14:17:06      Inj      : 1
                                                Inj Volume : 1 µl

Acq. Method    : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed   : 08.06.2022 14:22:28
Analysis Method : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed   : 20.06.2022 13:18:05
                (modified after loading)
Method Info    : 25.06.2019 H2
=====

```

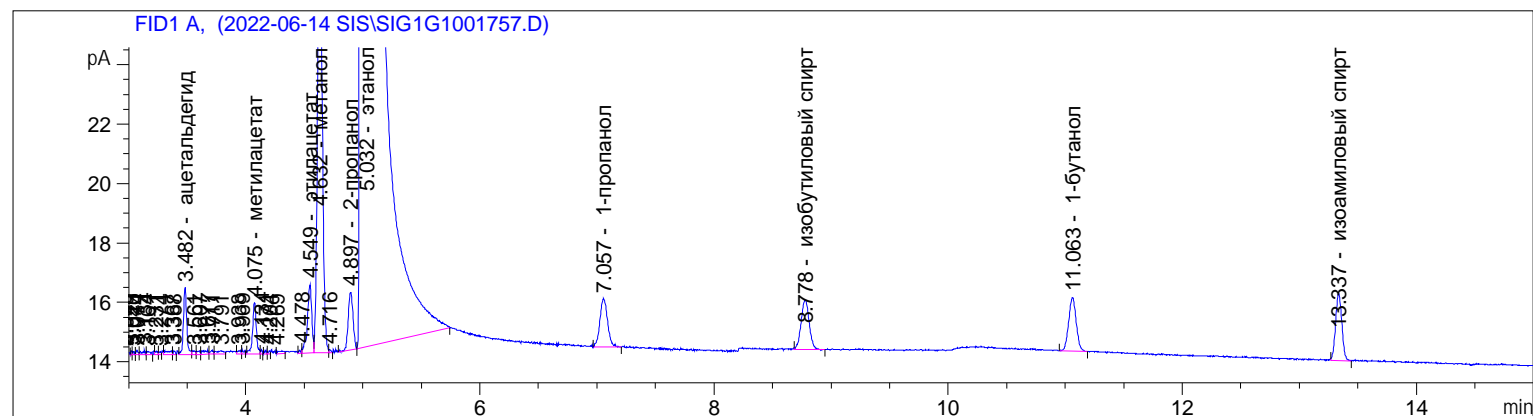

```

=====
Internal Standard Report
=====

```

```

Sorted By      :      Signal
Calib. Data Modified :      20 June 2022 г. 13:18:05
Multiplier:    :      1.0000
Dilution:      :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Sample ISTD Information:

ISTD ISTD Amount Name

```

#   мг/л безво
-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
1   7.89270e5   этанол

```

Signal 1: FID1 A,

RetTime [min]	Type	ISTD used	Area [pA*s]	Amt/Area ratio	Amount мг/л безво	Grp	Name
3.482	VV	1	4.35420	1.56500	26.63756		ацетальдегид
4.075	BV	1	3.88449	1.76261	26.76465		метилацетат
4.549	VV	1	5.88779	9.93171e-1	22.85851		этилацетат
4.632	VV	1	45.13608	1.41378e-4	2.49447e-2		метанол
4.897	VV	1	5.53714	9.40935e-1	20.36654		2-пропанол
5.032	VB S I	1	2.01908e5	1.00000	7.89270e5		этанол
7.057	VB	1	7.37778	7.03202e-1	20.28048		1-пропанол
8.778	BV	1	7.94120	6.29313e-1	19.53552		изобутиловый спирт
11.063	BV	1	8.10547	6.20938e-1	19.67426		1-бутанол
13.337	BV	1	8.35263	5.98564e-1	19.54367		изоамиловый спирт

Sample Name: pB

Totals without ISTD(s) : 175.68615

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

=====
*** End of Report ***