


Sample Name: calvados

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                Location : Vial 101
Injection Date  : 14.06.2022 12:38:52      Inj      : 1
                                           Inj Volume : 1 µl

Acq. Method     : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed    : 08.06.2022 14:22:28
Analysis Method : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed    : 20.06.2022 13:18:05
                 (modified after loading)
Method Info     : 25.06.2019 H2
=====

```

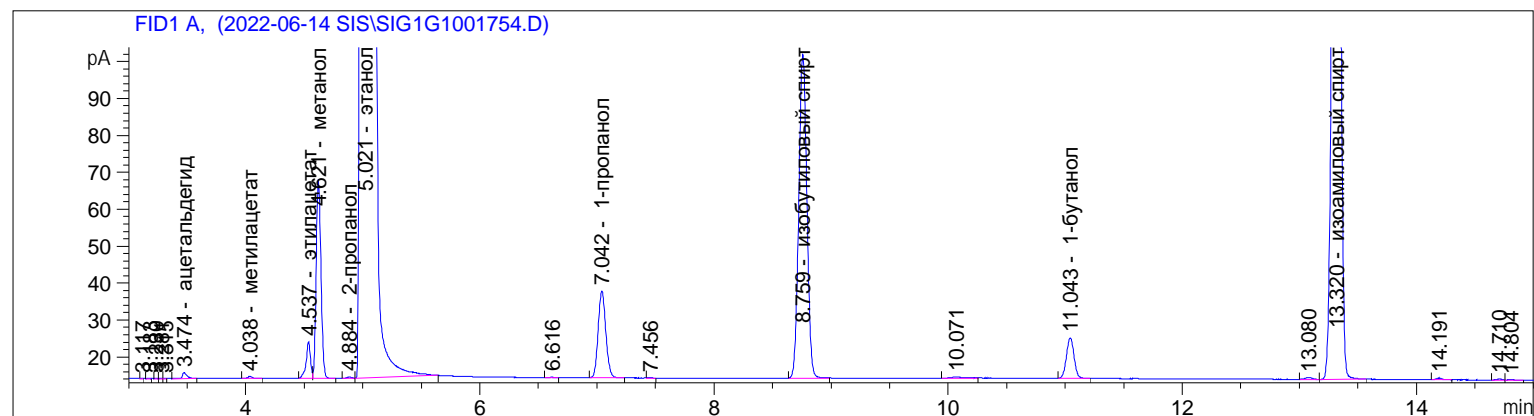

```

=====
Internal Standard Report
=====

```

```

Sorted By           :      Signal
Calib. Data Modified :      20 June 2022 г. 13:18:05
Multiplier:         :      1.0000
Dilution:           :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Sample ISTD Information:

ISTD ISTD Amount Name

# мг/л безво

```

-----|-----|-----|-----|-----|-----|-----|-----|-----|
1      7.89270e5      этанол

```

Signal 1: FID1 A,

RetTime [min]	Type	ISTD used	Area [pA*s]	Amt/Area ratio	Amount мг/л безво	Grp	Name
3.474	VB	1	4.37917	1.56500	25.90886		ацетальдегид
4.038	VB	1	1.29350	1.76261	8.61914		метилацетат
4.537	BV	1	25.59857	9.93171e-1	96.11284		этилацетат
4.621	VB	1	151.98273	1.41378e-4	8.12302e-2		метанол
4.884	BV	1	9.12064e-1	9.40935e-1	3.24434		2-пропанол
5.021	VB S I	1	2.08778e5	1.00000	7.89270e5		этанол
7.042	BB	1	106.46347	7.03202e-1	283.02355		1-пропанол
8.759	BB	1	422.47800	6.29313e-1	1005.10763		изобутиловый спирт
11.043	BB	1	49.52847	6.20938e-1	116.26381		1-бутанол
13.320	VB	1	1356.95068	5.98564e-1	3070.55167		изоамиловый спирт

Sample Name: calvados

Totals without ISTD(s) : 4608.91306

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

=====  
\*\*\* End of Report \*\*\*