


Sample Name: brendi

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                Location : Vial 101
Injection Date  : 14.06.2022 13:45:56      Inj      : 1
                                           Inj Volume : 1 µl

Acq. Method     : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed    : 08.06.2022 14:22:28
Analysis Method : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed    : 20.06.2022 13:18:05
                 (modified after loading)
Method Info     : 25.06.2019 H2
  
```

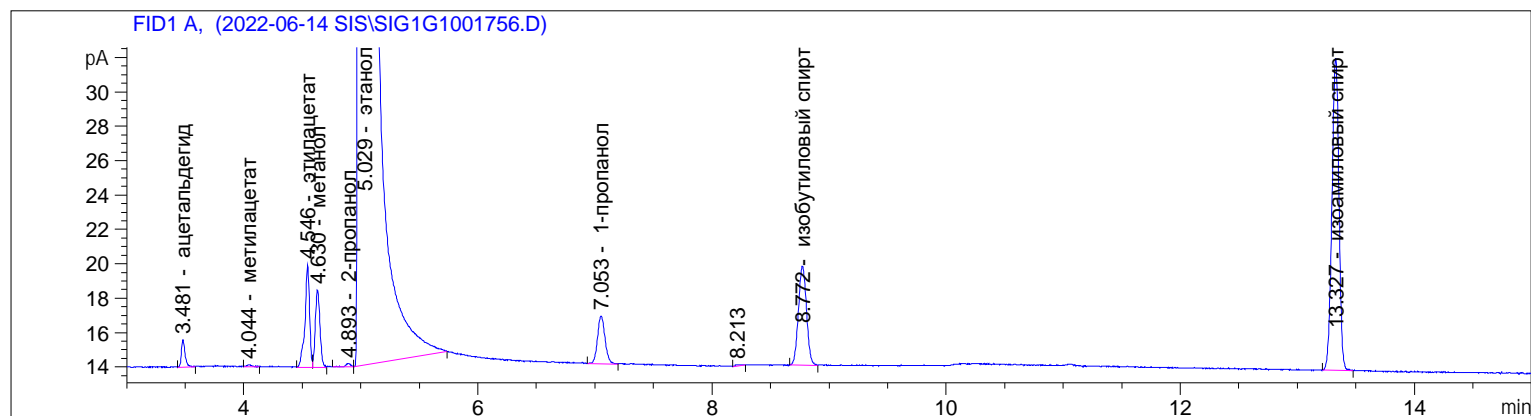

```

=====
Internal Standard Report
=====
  
```

```

Sorted By      : Signal
Calib. Data Modified : 20 June 2022 г. 13:18:05
Multiplier:    : 1.0000
Dilution:     : 1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Sample ISTD Information:

ISTD ISTD Amount Name

```

#   мг/л безво
-----|-----|-----
1   7.89270e5   этанол
  
```

Signal 1: FID1 A,

RetTime [min]	Type	ISTD used	Area [pA*s]	Amt/Area ratio	Amount мг/л безво	Grp	Name
3.481	VB	1	3.41524	1.56500	21.43389		ацетальдегид
4.044	VV	1	4.28908e-1	1.76261	3.03169		метилацетат
4.546	VV	1	16.22247	9.93171e-1	64.61099		этилацетат
4.630	VV	1	12.30149	1.41378e-4	6.97437e-3		метанол
4.893	VV	1	5.92681e-1	9.40935e-1	2.23638		2-пропанол
5.029	VB S I	1	1.96816e5	1.00000	7.89270e5		этанол
7.053	VB	1	12.50008	7.03202e-1	35.24994		1-пропанол
8.772	BV	1	27.64002	6.29313e-1	69.75424		изобутиловый спирт
11.026		1	-	-	-		1-бутанол
13.327	BV	1	75.29211	5.98564e-1	180.72808		изоамиловый спирт

Sample Name: brendi

Totals without ISTD(s) : 377.05220

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====

\*\*\* End of Report \*\*\*